

HORIBA

Micro Dilution Tunnel
MOLT-ONE
Partial Flow Dilution Sampling System



Explore the future

HORIBA

MDLT-ONE

The MDLT-ONE is designed to sample particulate emissions using the partial flow dilution method. A small portion of the total exhaust is diluted with HEPA* filtered air to create a constant flow rate through particulate filters to collect Particulate Matter (PM). Compliant to the latest regulations, the new MDLT-ONE is very compact and offers faster response by the use of high precision venturi flow meters and a piezo actuated valve.

* HEPA : High Efficiency Particulate Air

Features

- **Small package**

Heated filter system and flow controllers installed in a single rack. Swivel connection of tunnel section to cabinet allows flexible installation.

Auto filter changer* can also be mounted in the main rack for space efficiency.

- **Automatic calibration software enhances accuracy and ease of use**

The MDLT-ONE series performs automatic calibration by flowing air in-series through the two venturi flow meters and correcting any difference to zero in the software. This can be included into an automated sequence within a test template.

- **Integrated Operating Platform**


HORIBA ONE series systems employ a common user interface, "HORIBA ONE PLATFORM" offering future expandability and ease of integration into Test Automation Systems.




* Please contact HORIBA, when you ordering

Applications

PM Emission Measurement of All Engines

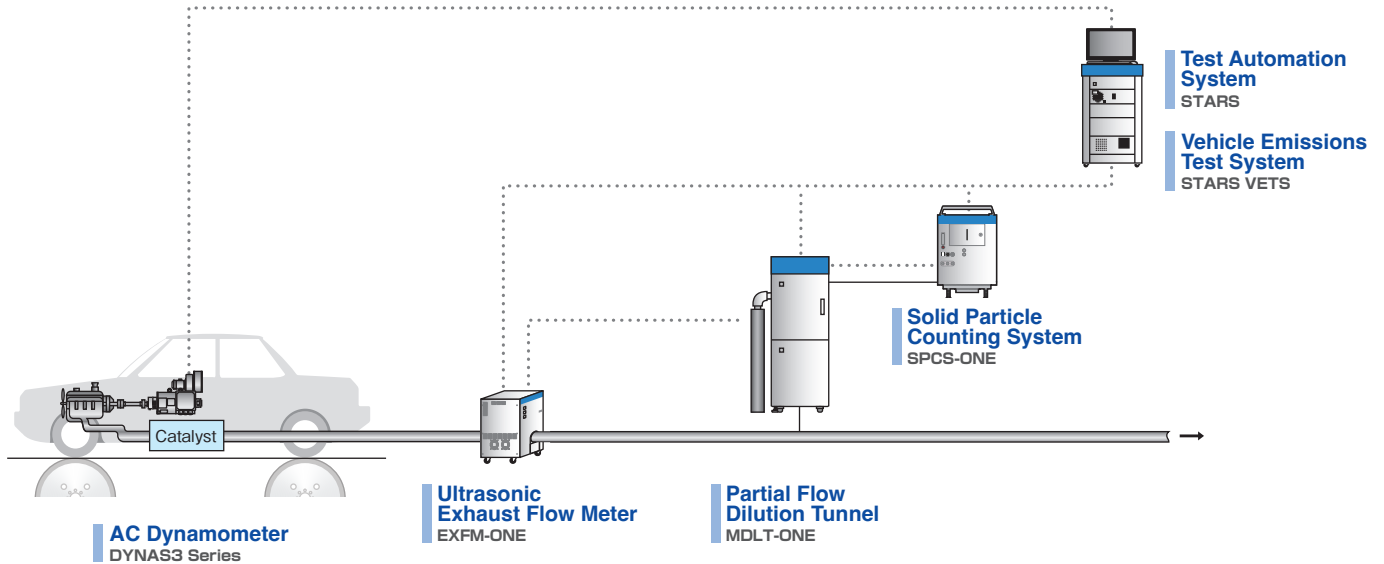

R&D Support of Engine and After Treatment System

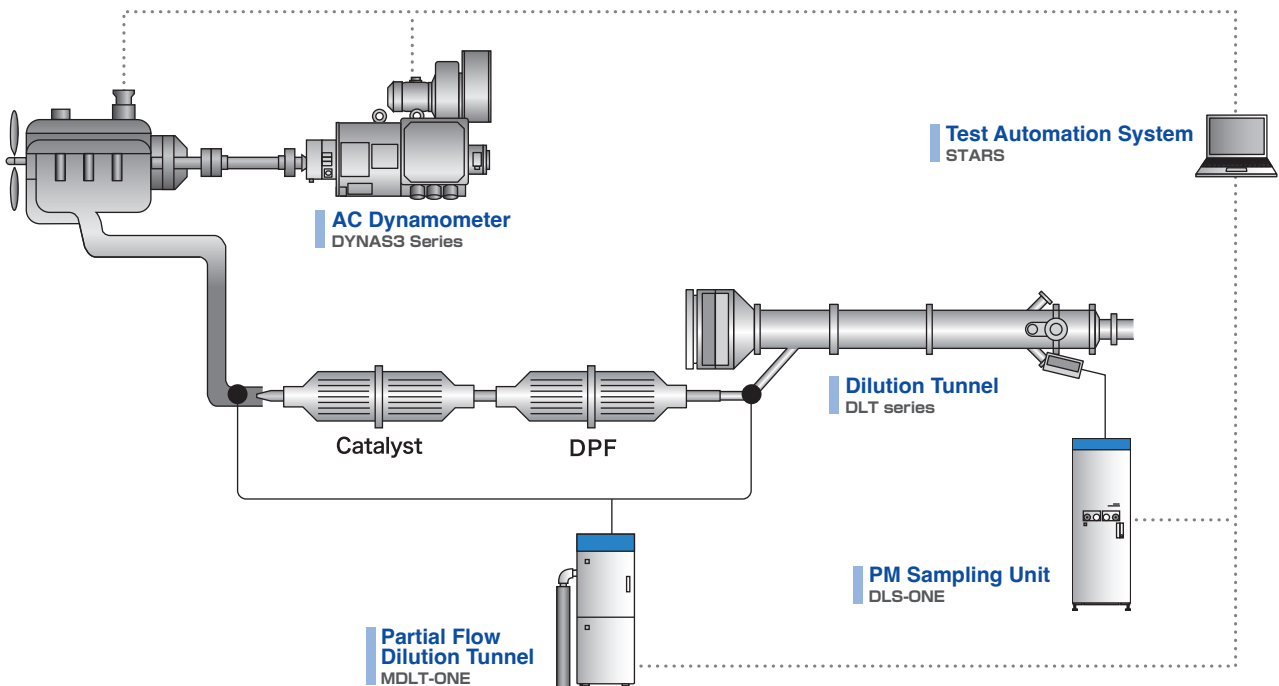

Complies with worldwide emissions regulations

ISO-16183

Japan: Post post new long term

EU: Euro VI (HDV)

EU: Stage IV / V (NRMM)

US: 40 CFR Part 1065/1066

Specification

System outline	
PM sampling method	Partial flow dilution method
Control modes for dilution	Proportional sampling mode (Const. split ratio)/ Fixed dilution ratio mode (Const. dilution ratio)/ Fixed flow rate mode (Manual control)
Control methods for dilution	- Real-time control based on analog input of exhaust flow rate - Control based on learned pattern of exhaust rate
Required signal for gas sampling	Isolated analog signal (0 to 10 V)
Flow rate of diluted gas	25 to 80 L/min* ¹ (under the condition of 20 °C and 101.3 kPa)
Accuracy of dilution ratio	Within ±5 % (Confirmed by measuring CO ₂) When dilution ratio=15 rate at 20 °C and 101.3 kPa : 53 to 80 L/min
PM mass calculation*²	PM mass (in g/test or g/kWh) can be calculated and saved, based on integrated values of flow rated and dilution ratio
Configurations	
System configuration	- Main unit : Dilution-tunnel unit - Operation unit : PC, monitor, keyboard and mouse (table is not included)
Utilities	Purified air : for dilution gas, 400 to 700 kPa, oil free, at least 100 L/min (at 20 °C and 101.3 kPa)
Power supply voltage and frequency	- Main unit : 100/110/120/200/220/230/240 V AC, 50/60 Hz, single phase - Operation unit : 100/110/120/200/220/230/240 V AC, 50/60 Hz, single phase
Power requirements	Main unit : Max. 3.0 kVA / Operation unit: Max. 0.5 kVA
Dimensions	- Main unit : 570 (W) x 730 (D) x 1700 (H) mm - Space for operation unit : 900 (W) x 500 (D) mm (table is not included)
Mass	Main unit : Approx. 300 kg (excluding operation unit)
Number of filter lines	Max. 6 lines (5 for sample, 1 for bypass)
Type of filter holder	- φ70 mm type : actual PM sampling area φ60 mm, with back-up filter - φ47 mm type : actual PM sampling area φ38.8 mm*¹, with back-up filter*¹
Operating conditions	
Sampling Pressure	Between atmospheric pressure and up to 40 kPa Back pressure of exhaust line : Less than 1 kPa
Options	
Filter auto-changer*³	Changer for automatic replacement of PM filter (φ 47 mm)
Valve switching	Additional air valve before filter (Replacement of sampling filter on bypass mode)
HOST interface*³	LAN communication using a 10 Base T port Conforms to IEEE802.3 (ISO880 2/3)
Conditioner for dilution air / Compressor	

*1, For the filter face velocity in the regulations (less than 100 cm/s), the flow rate for the φ47 mm filter must be 65 standard L/min.

*2, Input the amount of PM collected on filter to calculate PM mass. It is necessary to input engine output (kW) to calculate the PM mass engine output (g/kWh).

*3, Please contact HORIBA, when you ordering.



The HORIBA Group adopts IMS (Integrated Management System) which integrates Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System ISO45001.
We have now integrated Business Continuity Management System ISO22301 in order to provide our products and services in a stable manner, even in emergencies.



Please read the operation manual before using this product to assure safe and proper handling of the product.

- The specifications, appearance or other aspects of products in this catalog are subject to change without notice.
- Please contact us with enquiries concerning further details on the products in this catalog.
- The color of the actual products may differ from the color pictured in this catalog due to printing limitations.
- It is strictly forbidden to copy the content of this catalog in part or in full.
- The screen displays shown on products in this catalog have been inserted into the photographs through compositing.
- All brand names, product names and service names in this catalog are trademarks or registered trademarks of their respective companies.

<https://www.horiba.com/int/>

HORIBA, Ltd. Head Office 2 Miyanohigashi-cho, Kisshoin, Minami-ku, Kyoto, 601-8510, Japan Phone: 81 (75) 313-8121 Fax: 81 (75) 321-5725 Tokyo Sales Office 2-6, KandaAwaji-cho, Chiyoda-ku, Tokyo, 101-0063, Japan Phone: 81 (3) 6206-4721 Fax: 81 (3) 6206-4730	Japan	HORIBA India Private Limited 246, Okhla Industrial Estate, Phase 3 New Delhi-110020, India Phone: 91 (11) 4646-5000 Fax: 91 (11) 4646-5020 Technical Center D-255, Chakan MIDC Phase-II, Bhamboli Village, Pune-410501, India Phone: 91 (21) 3567-6000	India	HORIBA Test Automation Limited Brook Court Whittington Hall Worcester WR5 2RX, UK Phone: 44 (1905) 359-359 Fax: 44 (1905) 359-332	UK
HORIBA (China) Trading Co., Ltd. Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, 200335, Shanghai, China Phone: 86 (21) 6289-6060 Fax: 86 (21) 6289-5553 Beijing Branch 12F, Metropolis Tower, No.2, Haidian Dong 3 Street, Beijing, 100080, China Phone: 86 (10) 8567-9966 Fax: 86 (10) 8567-9066	China	HORIBA Instruments Incorporated 9755 Research Drive, Irvine, CA 92618, U.S.A. Phone: 1 (949) 250-4811 Fax: 1 (949) 250-0924 Ann Arbor Office 5900 Hines Drive, Ann Arbor, MI 48108, U.S.A. Phone: 1 (734) 213-6555 Fax: 1 (734) 213-6525	USA	HORIBA Europe Research Center 14 Boulevard Thomas Gobert - Passage Jobin Yvon CS 45002 - 91120 Palaiseau - France Phone: 33 (1) 69-74-72-00 Fax: 33 (1) 69-31-32-20	France
HORIBA (Thailand) Limited 46/8 Rungrojthanakul Bld., 1st, 2nd Floor, Ratchadapisek Road., Huai Khwang Bangkok 10310, Thailand Phone: 66 (0) 2861-5995 Fax: 66 (0) 2861-5200	Thailand	HORIBA Canada, Inc. Unit102, 5555 North Service Road Burlington, Ontario, Canada, L7L 5H7 Phone: 1 (905) 335-0234 FAX: 1 (905) 331-2362	Canada	HORIBA Europe GmbH Hans-Mess-Str.6, D-61440 Oberursel, Germany Phone: 49 (6172) 1396-0 Fax: 49 (6172) 1373-85	Germany
HORIBA KOREA Ltd. 25, 94-Gil, Iljik-Ro, Manan-Gu, Anyang-Si, Gyeonggi-Do, 13901, Korea Phone: 82 (31) 296-7911 Fax: 82 (31) 296-7913	Korea	TCA/HORIBA Sistemas de Testes Automotivos Ltda. Avenida Luigi Papaiz, 239 - Campanário, Diadema, São Paulo, Brazil CEP: 09931-610 Phone: 55 (11) 4224-0200 Fax: 55 (11) 4227-3133	Brazil	HORIBA ITALIA Srl Via Luca Gaurico 209 - 00143 ROMA Phone: 39 (6) 51-59-22-1 Fax: 39 (6) 51-96-43-34	Italy
		HORIBA (Austria) GmbH Kaplanstrasse 5, A-3430 Tulln, Austria Phone: 43 (2272) 65225 Fax: 43 (2272) 65225-45	Austria	HORIBA OOO Altufievskoe shosse, 13, building 5, 127106, Moscow, Russia Phone: 7 (495) 221-87-71 Fax: 7 (495) 221-87-68	Russia
		HORIBA UK Limited Kyoto Close Moulton Park Northampton NN3 6FL UK Phone: 44 (0) 1604-542500 Fax: 44 (0) 1604-542699	UK		