

ORGANIC POLLUTANT MONITOR OPSA-150

COD monitoring by UV absorption

Organic Pollutant Monitor

Measurement of Organic Matter
at Water Source

Measurement of Organic Matter
on the Process Line



Continuous Measurements
with Low Maintenance

Large Measurement Range
of 0 to 5.0 Abs



ORGANIC POLLUTANT MONITOR

OPSA-150



*Pole mount, outdoor cover, and analysis panel are available as options.

The OPSA-150 is a organic pollutant monitor that uses HORIBA's proprietary Rotary Cell Length Modulation, a measuring technique incorporating 25 years of expertise. The unit can be used as an organic pollutant monitor at drainage systems for determining compliance with COD monitoring regulations, for monitoring quality of water measuring levels of organic matter at water supply intakes, and as an organic monitor on process lines (phenol meter).


Sensor that makes full use of Rotary Cell Length Modulation

(JAPAN Patent No. 4627022
KOREA Patent No. 10-0840034
CHINA Patent No. ZL200610110930.8)

- Zero drift correction is performed in every cycle of measurement. This correction can eliminate the effect of any interference on cells.
- Cell length modulation provides readings from multiple measurements, making available results from various cell lengths. This allows the single device to make measurements on a large range of concentrations from as low as 0 to 0.1 Abs, up to 0 to 5.0 Abs.




Cell Length Modulation System

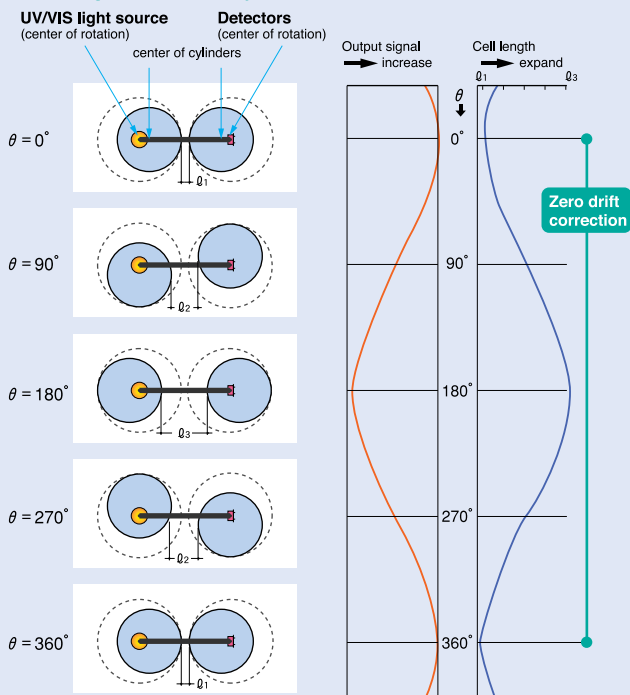

*CompactFlash is a registered trademark or trademark of SanDisk Corporation in the United States and other countries.

Easy-to-use Control Panel

Control of the OPSA-150 is operated via the intuitively designed touch panel. An interactive setup screen eliminates any doubts that a user may have while operating the unit. The Converted COD and TURB Display allow readings to be confirmed on site.

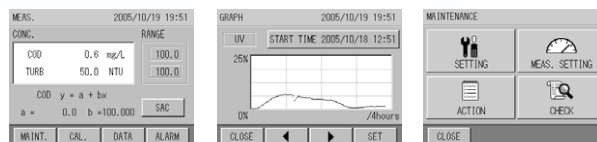

Automatic Data Recording up to One Year

Internal data memory provides data storage for one year in case of one measuring value per hour. A CompactFlash® card can be used to allow easy transfer of data to a PC.



HORIBA's Proprietary Wiper System

The cell is cleaned continuously by the wiper to eliminate any interference in the measurement light path. Therefore, errors in readings from dirty cells, or differences in results before and after cleaning are not evident.

Sample Failure Switch Input

The sample error alarm provided as an option on the previous OPSA-120 is now a standard feature.


Ten Times Increase in Analysis Sensitivity

The minimum accuracy of analysis ability has been increased to 0.0001 Abs, a ten-fold increase over the previous OPSA-120 unit. Measurements can be made on concentrations as low as 0 to 0.1 Abs.


Specifications

Name	Organic Pollutant Monitor	
Model name	OPSA-150	
Measurement items	UV absorbance, VIS absorbance, Converted COD level, Converted TURB level	
Principle	2 light path 2 wavelength cell length modulation rotary type	
Measurement wavelength	UV: 253.7 nm, VIS: 546.1 nm	
Construction of analysis section	Flow through type	
Range (Equivalent to a cell length of 10 mm)	UV absorbance / VIS absorbance 0 to 0.1 Abs - 0 to 5.0 Abs (Can be set 0.1 Abs increments)	
Resolution	0.0001 Abs (Can be set to 0.001 Abs)	
Repeatability	Within $\pm 2\%$ of full scale (within $\pm 5\%$ if full scale is 2.6 to 5.0 Abs)	
Linearity	Within $\pm 2\%$ of full scale (within $\pm 5\%$ if full scale is 2.6 to 5.0 Abs)	
Stability	Within $\pm 2\%$ of full scale in 24 hours (within $\pm 4\%$ in 24 hours if full scale is 2.6 to 5.0 Abs)	
Response time	T ₉₀ within 1 minute (flow rate of 5 L/min)	
Cleaning method (cleaning cycle)	Automatic cleaning via wipers (continuous cleaning)	
Display methods	LCD display: 320 x 240 monochrome crystal display with backlight (touch panel type) Display details: UV absorbance, VIS absorbance, UV-VIS absorbance (Absorbance can be changed to absorption constant (SAC: m ⁻¹), Converted COD level, Converted turbidity level	
Calibration method	Solution calibration (calibration solution inserted in ampule) via zero solution, span solution (single touch calibration)	
Sample conditions	Temperature: 2 to 40°C* Sample flow rate: Minimum 2 L/min, Maximum 20 L/min * Use a heating device to prevent sample freezing.	
Ambient conditions	Ambient temperature: 0 to 40°C, Ambient humidity: 85% or less	
Analog output	No. of outputs: 3 outputs (standard) Type: Up to 3 can be chosen from UV absorbance, VIS absorbance, UV-VIS absorbance, Converted COD level, and Converted TURB level outputs Specification: DC 4–20 mA, or DC 0–16 mA, isolated output (no isolation between each channel), maximum resistance load: 600 Ω	
Alarm and status outputs	No. of outputs: 6 outputs (standard) Type: Up to 4 can be chosen from power failure, maintenance (standard and fixed), batch alarm, COD maximum limit alarm, TURB limit alarm (standard), light source error, sample failure, cleaning motor error, and analyzer error outputs Details: Power failure...occurs when power fails Total alarm...cleaning motor error, light source error, analyzer error Maintenance...occurs when entering maintenance or correction mode, or when the maintenance switch has been turned on Specification: Dry contact output, NO contact Contact rating: AC 125 V 0.3 A, DC 30 V 1 A (with resistance load) Each output has an independent COM interface	
Contact input	No. of inputs: 2 inputs (standard) Type: Sample failure float switch input, time correction input Specifications: No-voltage contact input (can connect to open collector), isolated input On resistance: Maximum 100 Ω , Open voltage: DC 5.5 V, Short circuit current: 10 mA	
Communication	Interface: RS-232C Compatible Communication speed: 19200 bps	
Data memory	Values of measurement items are stored in the main unit's data memory. Data can also be transferred to a CompactFlash® card. Memory interval: 1 minute or 1 hour Memory save time: Every hour* Data memory capacity: 1 minute intervals...for 10 day's data, 1 hour intervals...for 1 year's data * The most recent data is saved to memory.	
Light source / Detector	Light source: Low pressure mercury lamp / Detector: Silicon photo cell	
Tubing connections	Sample entry: Rp-1/2 socket Bypass outlet: Rc-1/2 socket Overflow outlet (2): 20 A nominal diameter socket Overflow outlet (1): 13 A nominal diameter socket Drain outlet: 50 A nominal diameter socket Drain outlet: Rc-1/2 socket	
Construction	For outdoor installation	
Material of parts in contact with sample	SUS, PVC, PP, CR, SiO ₂	
Power source	AC 100 V to AC 230 V $\pm 10\%$, 50/60 Hz	
Power consumption	AC 100 V to AC 120 V: 45 VA maximum AC 200 V to AC 230 V: 60 VA maximum	
Weight	Operating section: Approx. 5.0 kg Analyzer section: Approx. 5.6 kg	
External dimensions	Operating section: 240 (W) x 104 (D) x 320 (H) Analyzer section: 200 (W) x 180 (D) x 403 (H) (units: mm) (excludes protruding sections)	
Color/Finish	Munsell 5PB8/1	
Installation conditions	● Install on a flat stable surface away from sources of vibration and shocks. ● Ambient air must not contain dust, mist or corrosive gases. ● Use at atmospheric pressure. ● Out of direct sunlight. ● An area with good air circulation. ● An altitude of less than 2000 m.	

■ Dimensional Outline (Unit: mm)

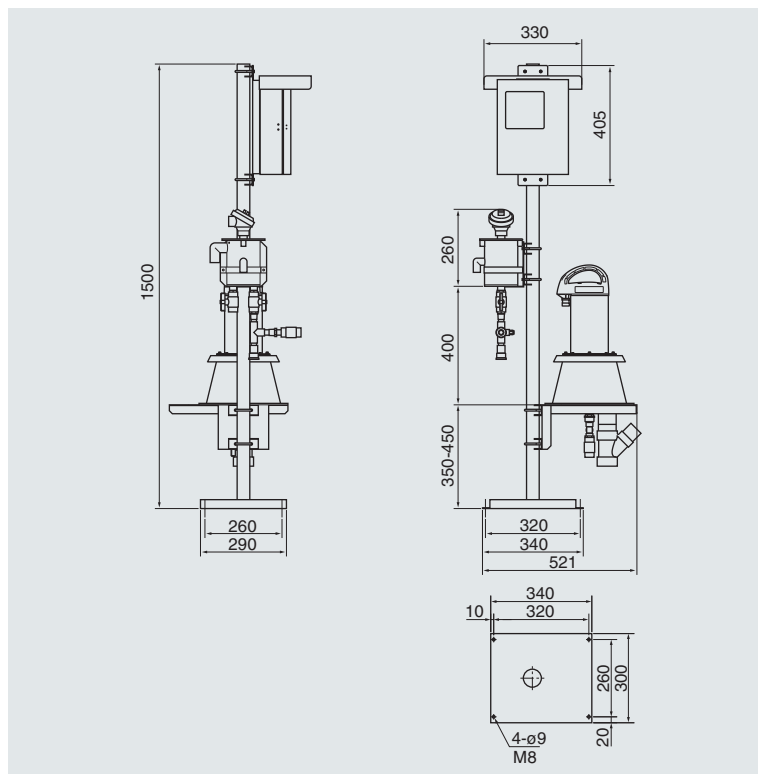

■ OPSA-150 Controller (Signals list)

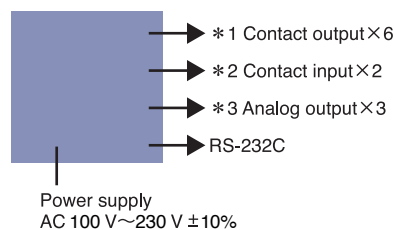

Signal name	Circuit	Standard
* 1 Contact output		●Max. switching voltage and current AC 125 V 0.3 A DC 30 V 1 A (Resistance load) ●No voltage contacts
* 2 Contact input		●No voltage contacts ●Isolated inputs [(-) common] ●ON resistance Max. 100 Ω ●Open voltage Max. DC 26 V ●Short circuit current Max. 13 mA
* 3 Analog output		●DC 4 - 20 mA current output ●Isolated output (COM common) ●Load resistance Max. 600 Ω

IMS

The HORIBA Group adopts IMS (Integrated Management System) which integrates Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System OHSAS18001. We have now integrated Business Continuity Management System ISO22301 in order to provide our products and services in a stable manner, even in emergencies.



Please read the operation manual before using this product to assure safe and proper handling of the product.

- The specifications, appearance or other aspects of products in this catalog are subject to change without notice.
- Please contact us with enquiries concerning further details on the products in this catalog.
- The color of the actual products may differ from the color pictured in this catalog due to printing limitations.
- It is strictly forbidden to copy the content of this catalog in part or in full.
- The screen displays shown on products in this catalog have been inserted into the photographs through compositing.
- All brand names, product names and service names in this catalog are trademarks or registered trademarks of their respective companies.

HORIBA

Head Office
2 Miyahonogashi-cho, Kisshoin Minami-ku, Kyoto, Japan
Phone: 81 (75) 313-8123 Fax: 81 (75) 321-5725
http://www.horiba.com e-mail: info@horiba.co.jp

Manufactured by
HORIBA Advanced Techno

HORIBA (China) Trading Co., Ltd. **China**

Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, Shanghai, 200335, China
Phone: 86 (21) 6289-6060 Fax: 86 (21) 6289-5553

Beijing Office

12F, Metropolis Tower, No.2, Haidian Dong 3 Street, Beijing, 100080, China
Phone: 86 (10) 8567-9966 Fax: 86 (10) 8567-9066

HORIBA (Thailand) Limited **Thailand**

East Office

850 / 7 Soi Lat Krabang 30 / 5, Lat Krabang Road, Lat Krabang, Bangkok 10520, Thailand
Phone: 66 (0) 2734 4434 Fax: 66 (0) 2734 4438

HORIBA Instruments (Singapore) Pte Ltd. **Singapore**

3 Changi Business Park Vista #01-01 Akzonobel House, Singapore 486051
Phone: 65 (6) 745-8300 Fax: 65 (6) 745-8155

HORIBA Vietnam Co., Ltd. **Vietnam**

Unit 6, 10 Floor, CMC Tower, Duy Tan Street, Dich Vong Hau Ward, Cau Giay District, Hanoi, Vietnam
Phone: 84 (24) 3795-8552 Fax: 84 (24) 3795-8553

PT HORIBA Indonesia **Indonesia**

Jl. Jalur Sutera Blok 20A, No.16-17, Kel. Kunciran, Kec. Pinang Tangerang-15144, Indonesia
Phone: 62 (21) 3044-8525 Fax: 62 (21) 3044-8521

HORIBA KOREA Ltd. **Korea**

25, 94-Gil, Iljik-Ro, Manan-Gu, Anyang-Si, Gyeonggi-Do, 13901, Korea
Phone: 82 (31) 296-7911 Fax: 82 (31) 296-7913

HORIBA India Private Limited **India**

246, Okhla Industrial Estate, Phase 3 New Delhi-110020, India
Phone: 91 (11) 4646-5000 Fax: 91 (11) 4646-5020

Technical Center

D-255, Chakan MIDC Phase-II, Bhamboli Village, Pune-410501, India
Phone: 91 (21) 3567-6000

Bangalore Office

No.55, 12th Main, Behind BDA Complex, 6th sector, HSR Layout, Bangalore South, Bangalore-560102, India
Phone: 91 (80) 4127-3637

HORIBA Instruments Incorporated **USA**

9755 Research Drive, Irvine, CA 92618, U.S.A.
Phone: 1 (949) 250-4811 Fax: 1 (949) 250-0924

Houston Office

5390 Bay Oaks Drive, Pasadena, TX 77505
Phone: 1 (281) 482-4334 Fax: 1 (281) 674-6058

HORIBA Instruments Brasil, Ltda. **Brasil**

Rua Presbitero Plinio Alves de Souza, 645, Parte A, Loteamento Multivias, Jardim Ermidia II - Jundiai Sao Paulo - CEP 13.212-181 Brazil
Phone: 55 (11) 2923-5400 Fax: 55 (11) 2923-5490

HORIBA Europe Research Center **France**

Avenue de la Vauve - Passage Jobin Yvon CS 45002 - 91120 Palaiseau - France
Phone: 33 (1) 69-74-72-00 Fax: 33 (1) 69-31-32-20

HORIBA UK Limited **UK**

Kyoto Close Moulton Park, Northampton NN3 6FL, UK
Phone: 44 (1604) 542-5000 Fax: 44 (1604) 542-699

HORIBA Europe GmbH **Germany**

Hans-Mess-Str.6 D-61440 Oberursel Germany
Phone: 49 (6172) 1396-0 Fax: 49 (6172) 1373-85

Leichlingen Office

Julius-kronenberg Str.9 D-42799 Leichlingen Germany
Phone: 49 (2175) 8978-0 Fax: 49 (2175) 8978-50

HORIBA Czech **Czech**

Prague Office

Prumyslova 1306 / 7, CZ-10200, Praha 10, Czech Republic
Phone: 420 (2) 460-392-65

HORIBA (Austria) GmbH **Austria**

Kaplanstrasse 5 A-3430 Tulln, Austria
Phone: 43 (2272) 65225 Fax: 43 (2272) 65230

HORIBA (Austria) GmbH **Romania**

Romania Branch
B-dul.Republicii, nr. 164, Etaj Parter, Birourile nr. 3 si 4 Pitestijudetul Arges110177 Romania
Phone: 40 (348) 807117 Fax: 40 (348) 807118